



Polymer Optical Fibre Bragg Grating Humidity Sensor at 100°C

Woyessa, Getinet; Fasano, Andrea; Markos, Christos; Rasmussen, Henrik K.; Bang, Ole

Published in:

Proceedings of the 25th International Conference on Plastic Optical Fibers 2016

Publication date:

2016

Document Version

Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

Citation (APA):

Woyessa, G., Fasano, A., Markos, C., Rasmussen, H. K., & Bang, O. (2016). Polymer Optical Fibre Bragg Grating Humidity Sensor at 100°C. In Proceedings of the 25th International Conference on Plastic Optical Fibers 2016 University of Aston in Birmingham.

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Polymer Optical Fibre Bragg Grating Humidity Sensor at 100°C

G. Woyessa^{1*}, A. Fasano², C. Markos¹, H.K. Rasmussen², O. Bang¹

1 DTU Fotonik, Department of Photonics Engineering, Technical University of Denmark, DK-2800 Kgs. Lyngby, Denmark

2 DTU Mekanik, Department of Mechanical Engineering, Technical University of Denmark, DK-2800 Kgs. Lyngby, Denmark

*Corresponding author: gewoy@fotonik.dtu.dk

Abstract: We have demonstrated a polymer optical fibre Bragg grating humidity sensor that can be operated up to 100°C. The sensor has been fabricated from a polycarbonate (PC) microstructured polymer optical fibre Bragg grating (mPOFBG). PC mPOFBG gave a relative humidity (RH) sensitivity of 6.95 ± 0.83 pm/% RH in the range 10-90% RH at 100°C and a temperature sensitivity of 25.94 ± 0.47 pm/°C in the range 20 - 100 °C at 90% RH. Despite PC mPOFBGs shows smaller humidity sensitivity compared to PMMA mPOFBGs, they can be used to sense humidity beyond the operating temperature limit of PMMA mPOFBGs.

Key Words: Polymer optical fibre, Fibre Bragg grating, Fibre optic sensor, Humidity sensor, Annealing.

1. Introduction

The interest in polymer optical fibres (POFs) in sensing is steadily increasing because of their low processing temperature, high flexibility in bending, high fracture toughness, ease of handling, and non-brittle nature, which are properties that glass fibres do not have [1-2]. In addition, POFs are biocompatible and have a high elastic strain limit and low Young's modulus, which makes them advantageous for fibre Bragg grating (FBG) based strain and bio-sensing applications [3-5]. Some polymers, such as PMMA, are humidity sensitive and strongly absorb water [6], while other polymers, such as TOPAS 5013, were shown to be insensitive to humidity and high operating temperature [7]. Nevertheless, it is polycarbonate microstructured polymer optical fibre (mPOF) that has the highest operating temperature among currently existing POFs [8]. Due to the moisture absorbing capability of PMMA based POFs, which leads to a change in the refractive index and size of the fibre, both of which contribute to a change in Bragg wavelength [9], they are used for developing humidity sensors [10]. PC has also moisture absorbing capability although it is smaller than that of PMMA. The water absorption (saturation value) at 23°C of PC is 0.3% [11], and PMMA is 2.1% [12]. This means that the water absorption capability of PC is 7 times smaller than that of PMMA but about 40°C larger glass transition temperature (T_g) as compared to PMMA.

For PMMA POFBGs the temperature operational limit is strongly dependent on the surrounding relative humidity (RH) level at which they are being operated, in addition to its T_g . If they are operated at ambient or less RH level, this limit is 15-20°C below their T_g . For instance, at ambient RH PMMA POFBGs has been operated up to 90 °C [13]. But, when the surrounding RH is high, the temperature operational limit significantly decreases. For instance, at 90% RH they can be operated only up to 75 °C [14]. This is due to the fact that for such polymers the glass transition temperature decreases with increasing humidity. Similarly, when PMMA POFBGs are used as humidity sensor the RH range of operation highly dependent on the temperature of the environment in which the sensors are being operated. PMMA POFBG has been operated from 10-90% RH up to 75°C. However, beyond this temperature the grating could not handle it. If the temperature in which PMMA POFBGs humidity sensors are being operated is higher than 75°C, the maximum RH should be less than 90%. For instance, if we want to operate PMMA POFBGs at 85 °C, the range of RH operation will be limited to only 60% RH for stable operation. Likewise, at 90°C the range of possible RH becomes even narrower. Thus, it is important to develop POFBG humidity sensors which can operate at high temperature and also with wide range of RH for some applications. Here we demonstrated a stable and highly linear mPOFBGs humidity sensor that can be operated beyond 100°C and with RH range of up to 90%. This sensor is developed with PC mPOFBGs.

2. Experiment

The fibre used in this experiment is a PC mPOF. The diameter of the fiber is $130\mu\text{m}$, and the hole and the pitch size are $1.5\mu\text{m}$ and $4.2\mu\text{m}$, respectively. The hole to pitch ratio is 0.38, ensuring that the fiber is endlessly single mode [15]. First FBG was inscribed by using phase mask technique. The setup used was the same as described in ref. 16. The Bragg wavelength of the grating was 892.67nm and the full width half maximum was 0.8nm . The PC mPOFBG was first connectorized [17] and coupled with a single mode silica fibre and then placed in the CLIMACELL environmental chamber. A Supercontinuum source (NKT Photonics A/S) has been used as a light source and Compact CCD Spectrometer (THORLABS) has been used to continuously track the grating in the chamber during the experiment. The FBG has been first annealed at 100°C and 90% relative humidity (RH). The annealing process was stopped when the rate of blue shift was less than $0.1\text{nm}/\text{hour}$. This process took 26 hours. The amount of blue shift was 8nm .

After annealing the humidity response of the mPOFBG sensor has been measured at 100°C in the interval of 10-90% RH. At this temperature and RH range the environmental chamber has a precision of 0.5°C and 1% RH. The humidity measurement has been done first by increasing the RH from 10% to 90%, with step of 10% and then decreasing it from 90% to 10% with step of 10%. The stabilization period after incrementing or decrementing the RH was 60 minutes.

We have also measured the temperature sensitivity at 90% RH in the range 20 to 100°C . The temperature measurement has been done first by increasing the temperature from 20 to 100°C , with steps of 10°C and then decreasing it back to 20°C with same amount of step. The stabilization period after incrementing or decrementing the temperature was 60 minutes.

3. Results

The response of the PC mPOFBGs for both increasing and decreasing relative humidity at 100°C for the stabilized period is shown in Fig. 1.

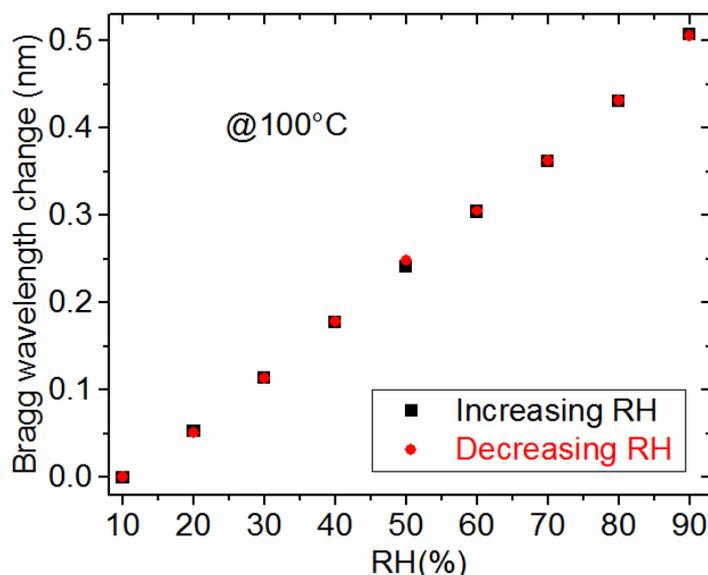


Figure 1. Measured humidity response at 100°C of the PC mPOFBG.

The humidity sensitivity at 100°C was 6.95 ± 0.83 pm/%RH for both increasing and decreasing humidity. The R-squared for this fitted regression line is 0.998. The humidity sensitivity of a PMMA mPOFBG at 75 °C, which is the maximum operating temperature at higher RH, in the 850nm region is typically around 45 pm/%RH in the range 10-90%. This shows that PC mPOFBG has wider operating temperature range but lower RH sensitivity as compared to PMMA mPOFBGs.

The response of the PC mPOFBGs for both increasing and decreasing temperature at 90% RH is shown in Fig. 2. The temperature sensitivity at 90 % RH was 25.94 ± 0.47 pm/°C for both increasing and decreasing temperature. The R-squared for this fitted regression line is 0.998. There were no hysteresis observed for both humidity and temperature measurement. This is due to the fact the FBG was annealed well enough.

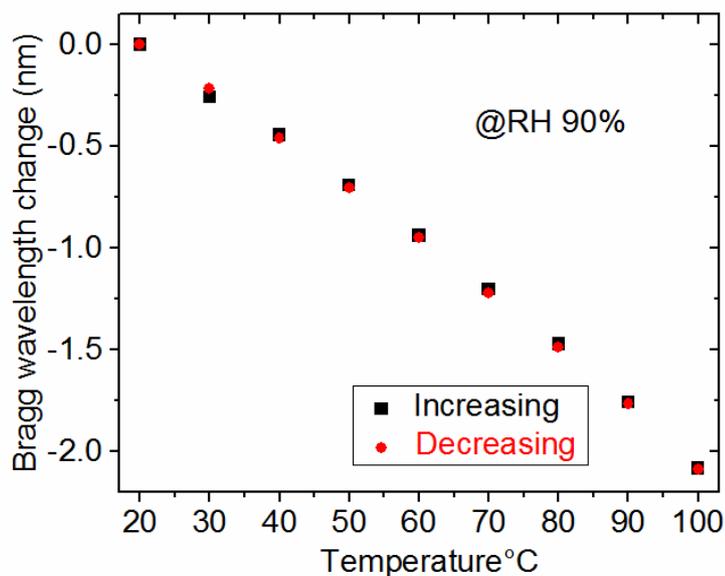


Figure 2. Measured temperature response at 90% RH of the PC mPOFBG.

4. Conclusion

We have developed a polymer optical fibre Bragg grating humidity sensor that can be operated up to 100°C. The sensor has been fabricated from a PC mPOFBG. PC mPOFBG gave a RH sensitivity of 6.95 ± 0.83 pm/%RH in the range 10-90% RH at 100°C and a temperature sensitivity of 25.94 ± 0.47 pm/°C in the range 20-100 °C at 90% RH. Thus, PC mPOFBGs humidity sensors can be used beyond the operating temperature limit of PMMA mPOFBGs.

Acknowledgments

The research leading to these results has received funding from the People Programme (Marie Curie Actions) of the European Union's Seventh Framework Programme FP7/2007-2013/ under REA grant agreement n° 608382.

References

- [1].K. Peters, "Polymer optical fiber sensors - A review," *Smart Mater. Struct.* **20**(1), 013002 (2011).
- [2].H. Dobb, D. J. Webb, K. Kalli, A. Argyros, M. C. J. Large, and M. A. van Eijkelenborg, "Continuous wave ultraviolet light-induced fiber Bragg gratings in few- and single-mode microstructured polymer optical fibers," *Opt. Lett.* **30**(24), 3296–3298 (2005).

- [3].Z. Xiong, G. D. Peng, B. Wu, and P. L. Chu, "Highly tunable Bragg gratings in single-mode polymer optical fibers," IEEE Photon. Technol. Lett. **11**(3), 352–354 (1999).
- [4].H.Ul Hassan, K.Nielsen, S.Aasmul, and O.Bang, "Polymer optical fiber compound parabolic concentrator tip for enhanced coupling efficiency for fluorescence based glucose sensors", Bio.Opt. Express **12**(2), 5008–5020 (2015).
- [5].C.Broadway, D.Gallego, G.Woyessa, A.Pospori, G.Carpintero, O.Bang, K.Sugden, and H.Lamela, "Fabry-Perot microstructured polymer optical fiber sensors for opto-acoustic endoscopy", Proc. SPIE **9531**, 953116 (2015).
- [6].C. Zhang, W. Zhang, D. J. Webb, and G. D. Peng, "Optical fiber temperature and humidity sensor," Electron. Lett. **46**(9), 643–644 (2010).
- [7].C. Markos, A. Stefani, K. Nielsen, H. K. Rasmussen, W. Yuan, and O. Bang, "High-Tg TOPAS microstructured polymer optical fiber for fiber Bragg grating strain sensing at 110 degrees, " Opt. Express **21**(4), 4758–4765 (2013).
- [8].A.Fasano, G.Woyessa, P.Stajanca, C. Markos, A.Stefani, K.Nielsen, H. K. Rasmussen, K. Krebber, and O. Bang, "Fabrication and characterization of polycarbonate microstructured polymer optical fibers for high-temperature-resistant fiber Bragg grating strain sensors" Opt. Mater. Express, **6**(2), 649-659(2016).
- [9].N. G. Harbach, "Fiber Bragg gratings in polymer optical fibers," PhD Thesis, Lausanne, EPFL (2008).
- [10].Z. F. Zhang and X. M. Tao, "Synergetic effects of humidity and temperature on PMMA based fiber Bragg gratings," J. Lightwave Technol. **30**(6), 841–845 (2012).
- [11].<http://www.plastics.covestro.com/en/Products/Makrolon/ProductList/201305212210/Makrolon-LED2245>
- [12].<http://www.gehrplastics.com/pmma-acrylic.html>
- [13].K. E. Carroll, C. Zhang, D. J. Webb, K. Kalli, A. Argyros, and M. C. J. Large, "Thermal response of Bragg gratings in PMMA microstructured optical fibers," Opt. Express **15**(14), 8844–8850 (2007).
- [14].G.Woyessa, K.Nielsen, A.Stefani, C.Markos and O.Bang, "Temperature insensitive hysteresis free highly sensitive polymer optical fiber Bragg grating humidity sensor", Opt. Express **24**(2), 1206-1213 (2016).
- [15].T. A. Birks, J. C. Knight, and P. St.J. Russell, "Endlessly single-mode photonic crystal fiber," Opt. Lett. **22**(13), 961–963 (1997).
- [16].I.-L. Bundalo, K. Nielsen, C. Markos, and O. Bang, "Bragg grating writing in PMMA microstructured polymer optical fibers in less than 7 minutes," Opt. Express **22**(5), 5270–5276 (2014).
- [17].A. Abang and D. J. Webb, "Demountable connection for polymer optical fiber grating sensors," Opt. Eng. **51**(8), 080503-1 (2012).