



## Contact area measurements on structured surfaces

Kücükyildiz, Ömer Can; Jensen, Sebastian Hoppe Nesgaard; De Chiffre, Leonardo

*Publication date:*  
2016

*Document Version*  
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

*Citation (APA):*  
Kücükyildiz, Ö. C., Jensen, S. H. N., & De Chiffre, L. (2016). Contact area measurements on structured surfaces. Poster session presented at Euspen's S.I.G. Meeting, Copenhagen, Denmark.

## DTU Library

Technical Information Center of Denmark

---

### General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.



# Contact area measurements on structured surfaces



Ömer C. Kücükıldız, Sebastian H. N. Jensen, Leonardo De Chiffre

Department of Mechanical Engineering and Department of Applied Mathematics and Computer Science,  
Technical University of Denmark






In connection with the use of brass specimens featuring structured surfaces in a tribology test, an algorithm was developed for automatic measurement of the contact area by optical means.

The contact area of the specimen after deformation is visible on a digital photograph as 10 parallel bands in adequate contrast to the background.

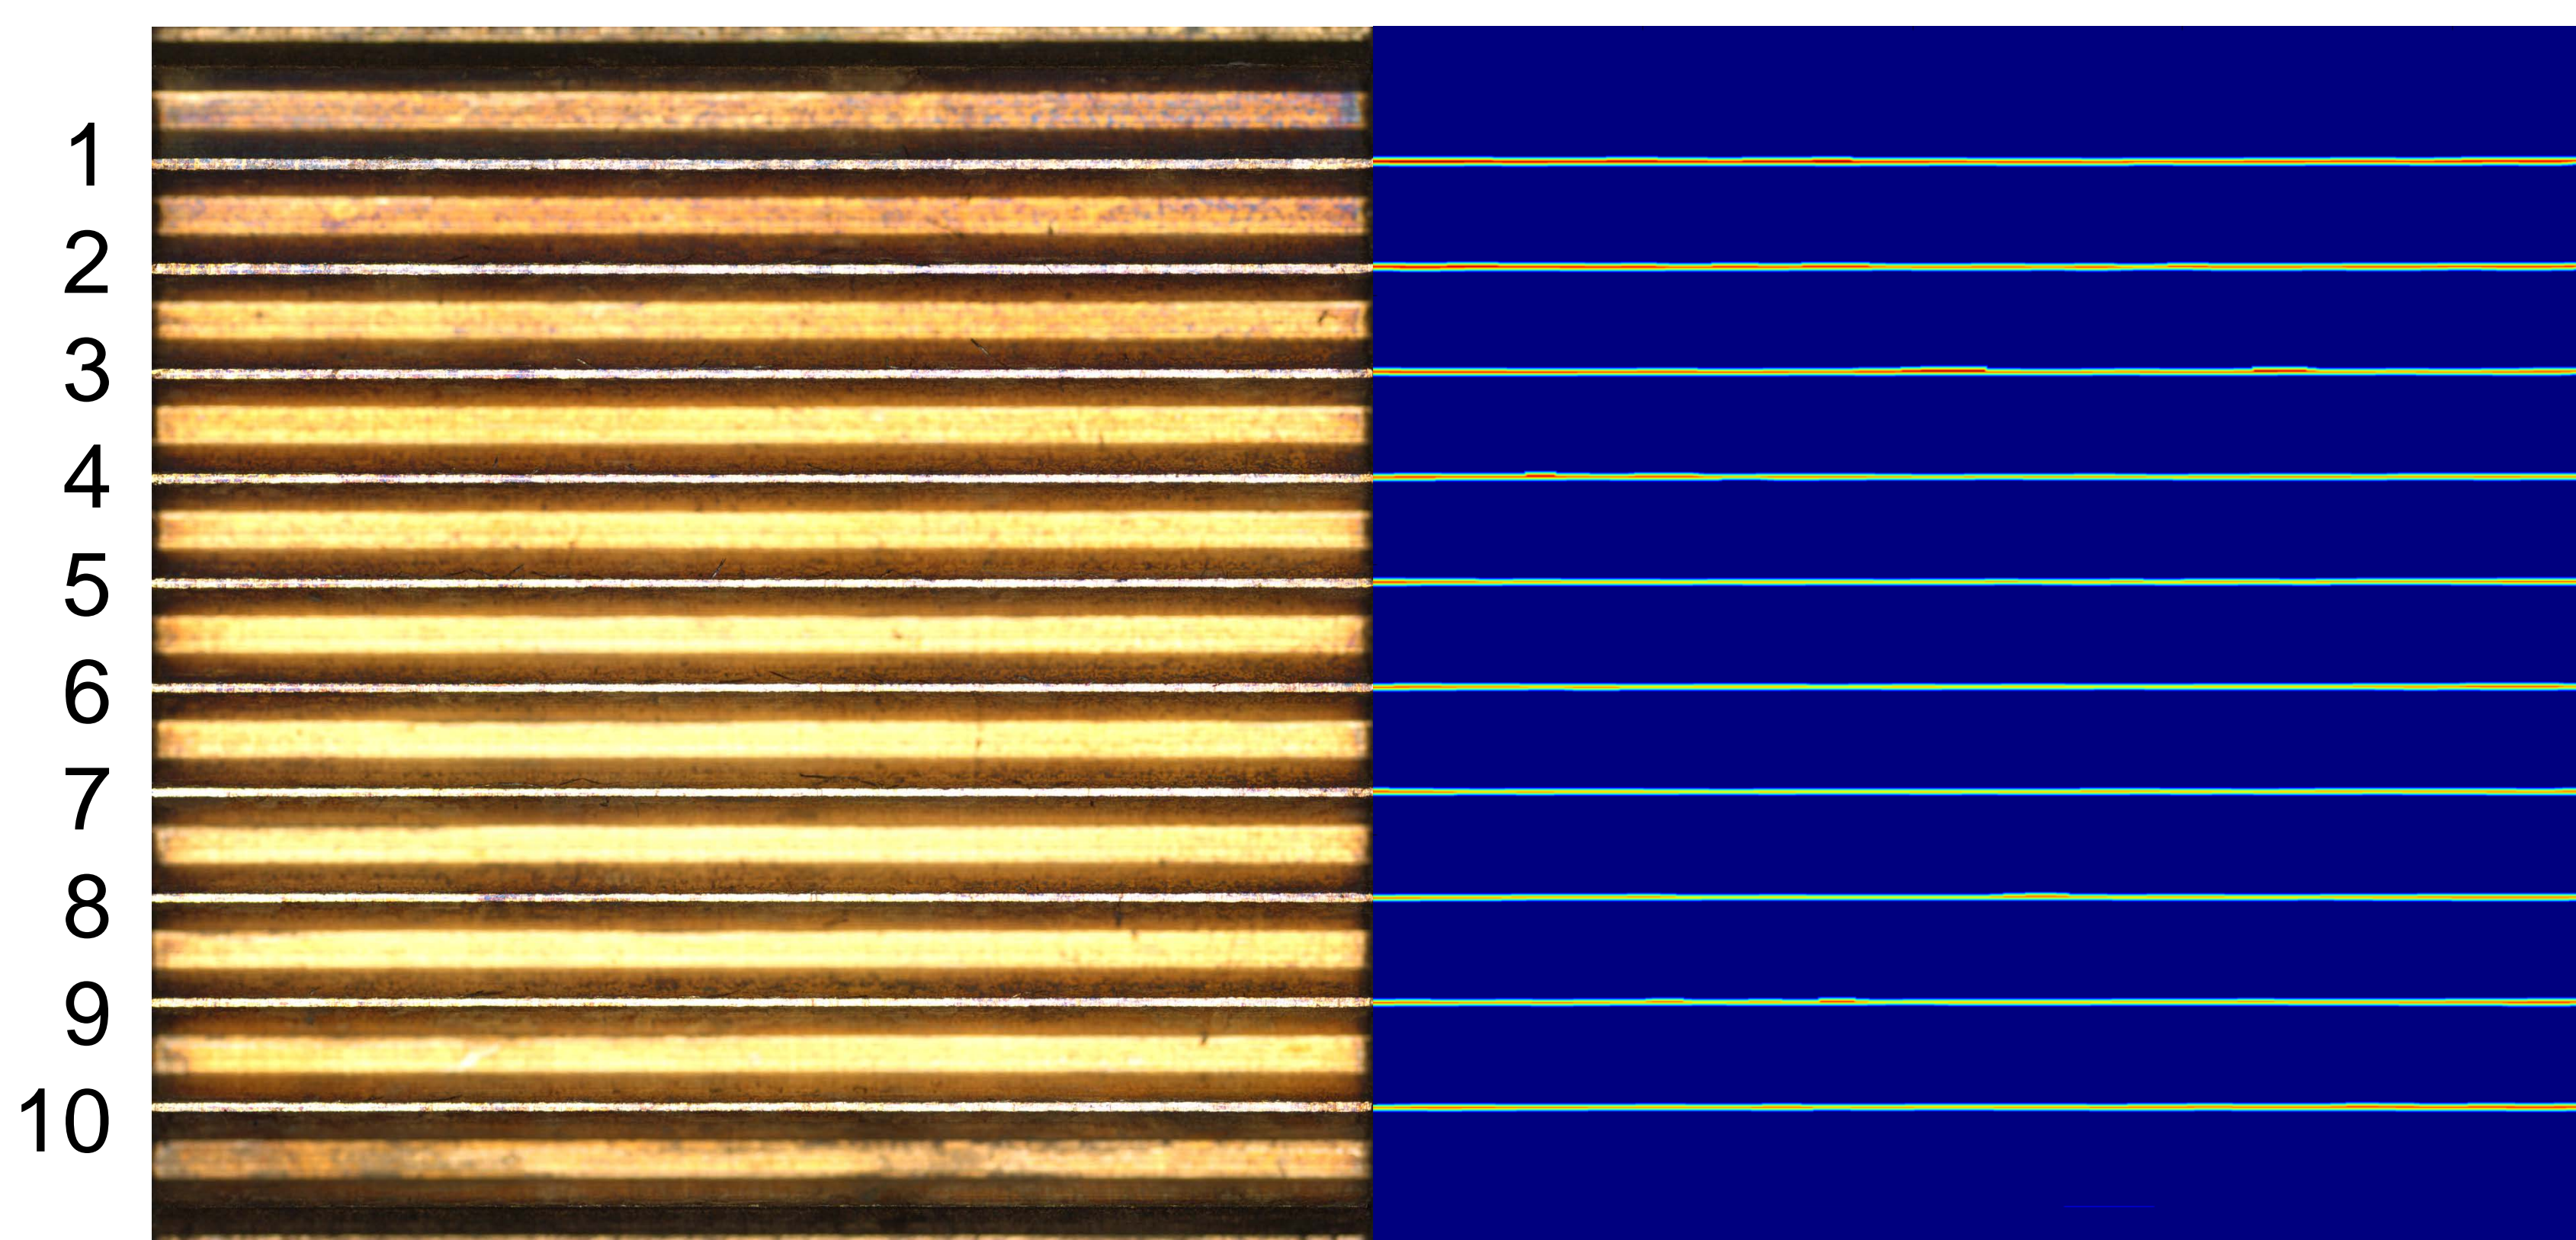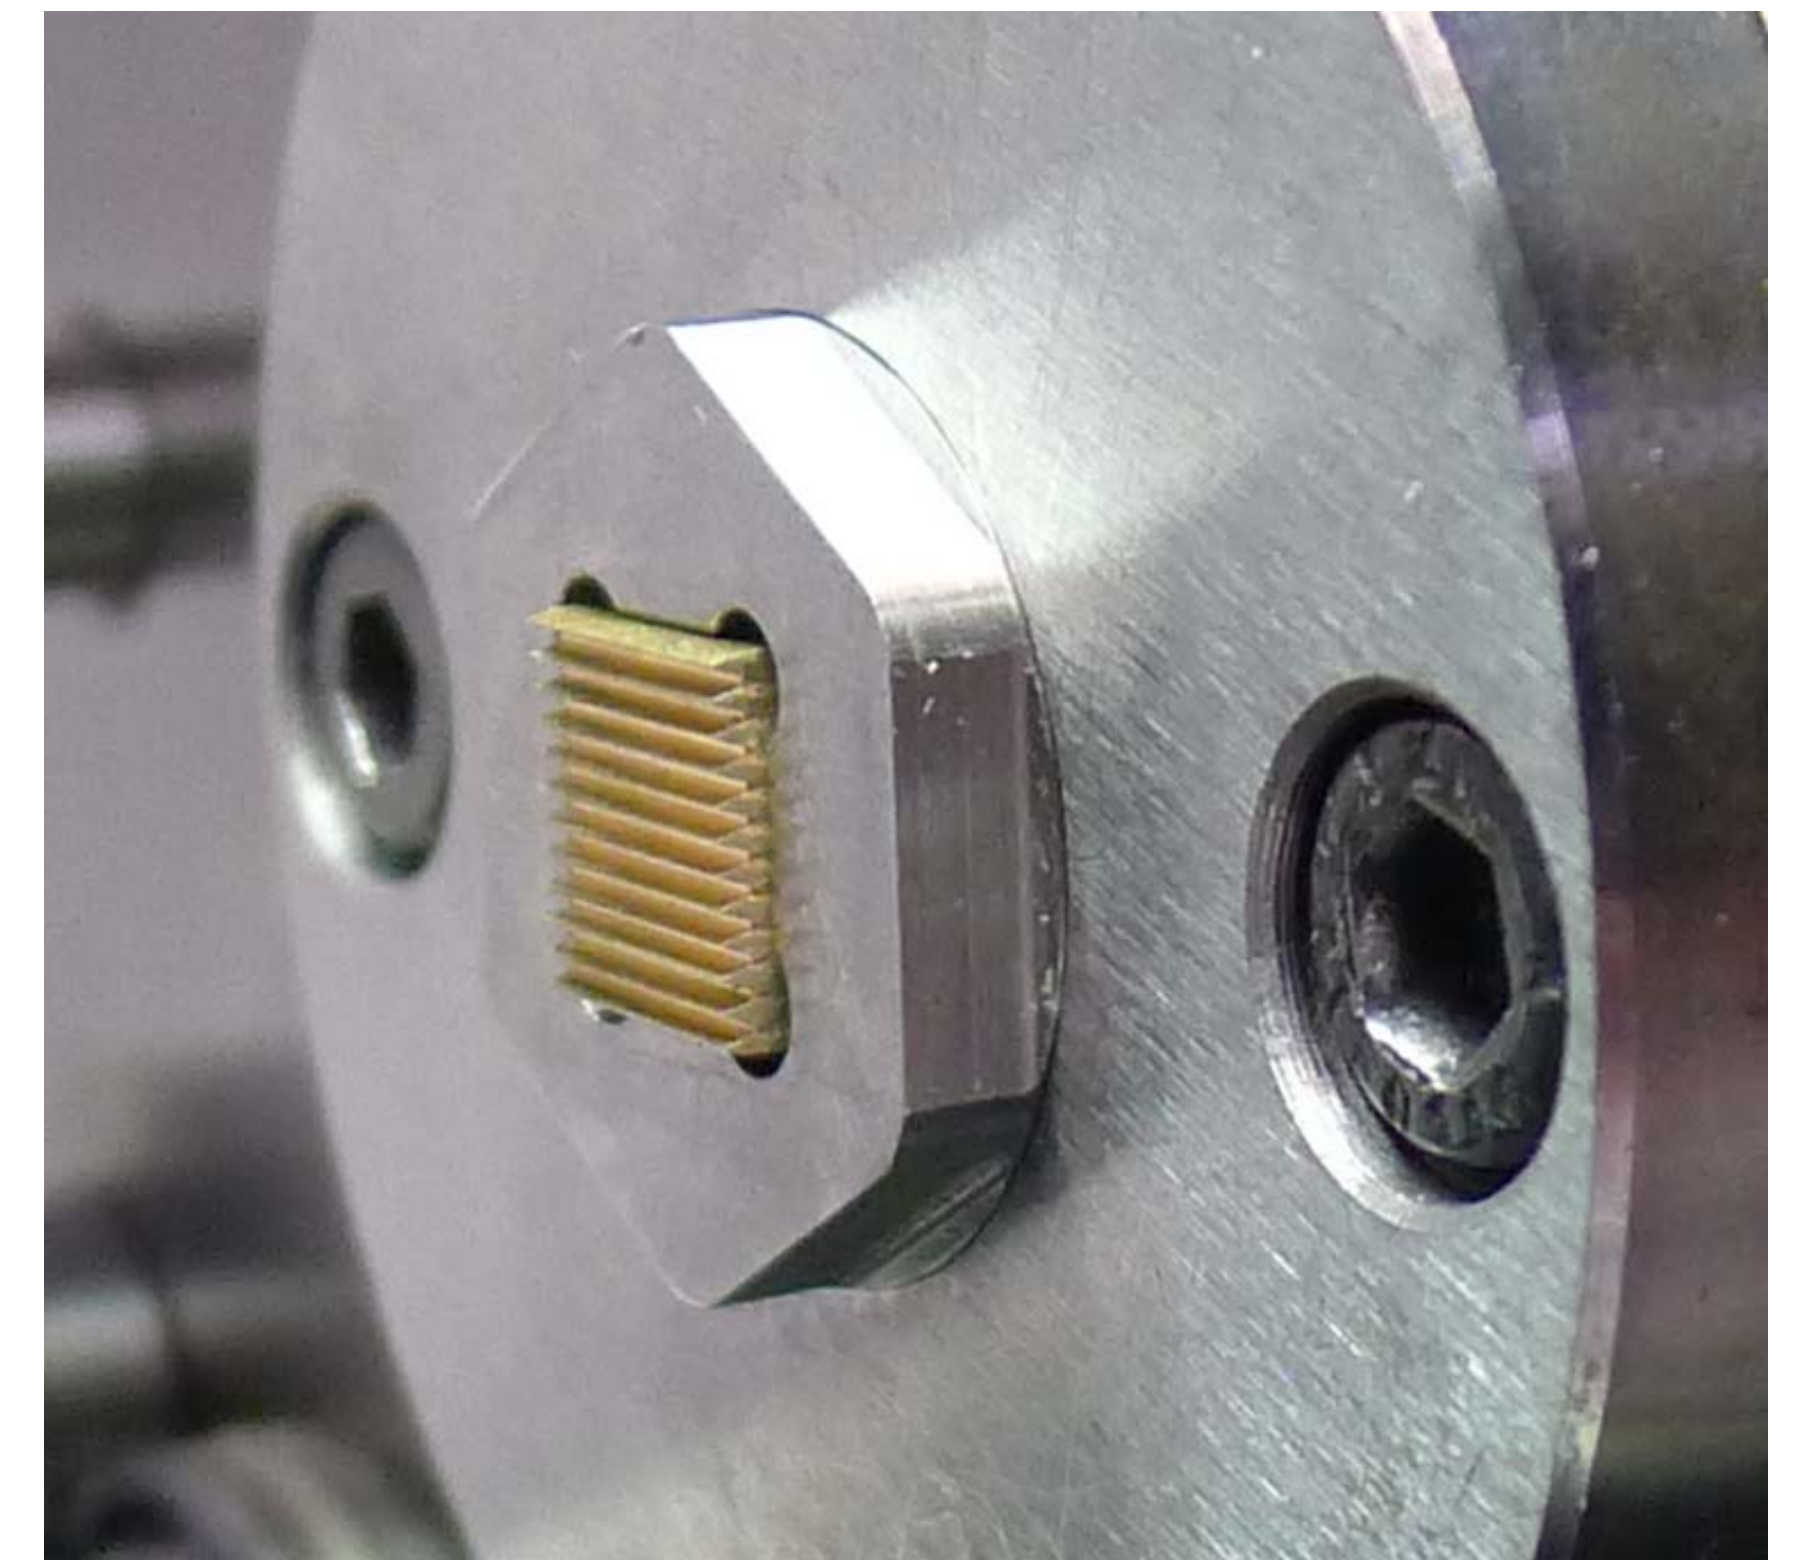

An approach was developed that automatically performs a pixel segmentation based on local image gradient extrema, leading to an accurate band-edge segmentation. For each band, a fine-grained line width is estimated through the distance transform in conjunction with non-max suppression, which can be used to estimate the desired area statistics.

During this study, the traceability of the method was established through an optical standard from NPL. Measuring line-widths in the range 10-100  $\mu\text{m}$ , errors less than 0.4  $\mu\text{m}$  were obtained.

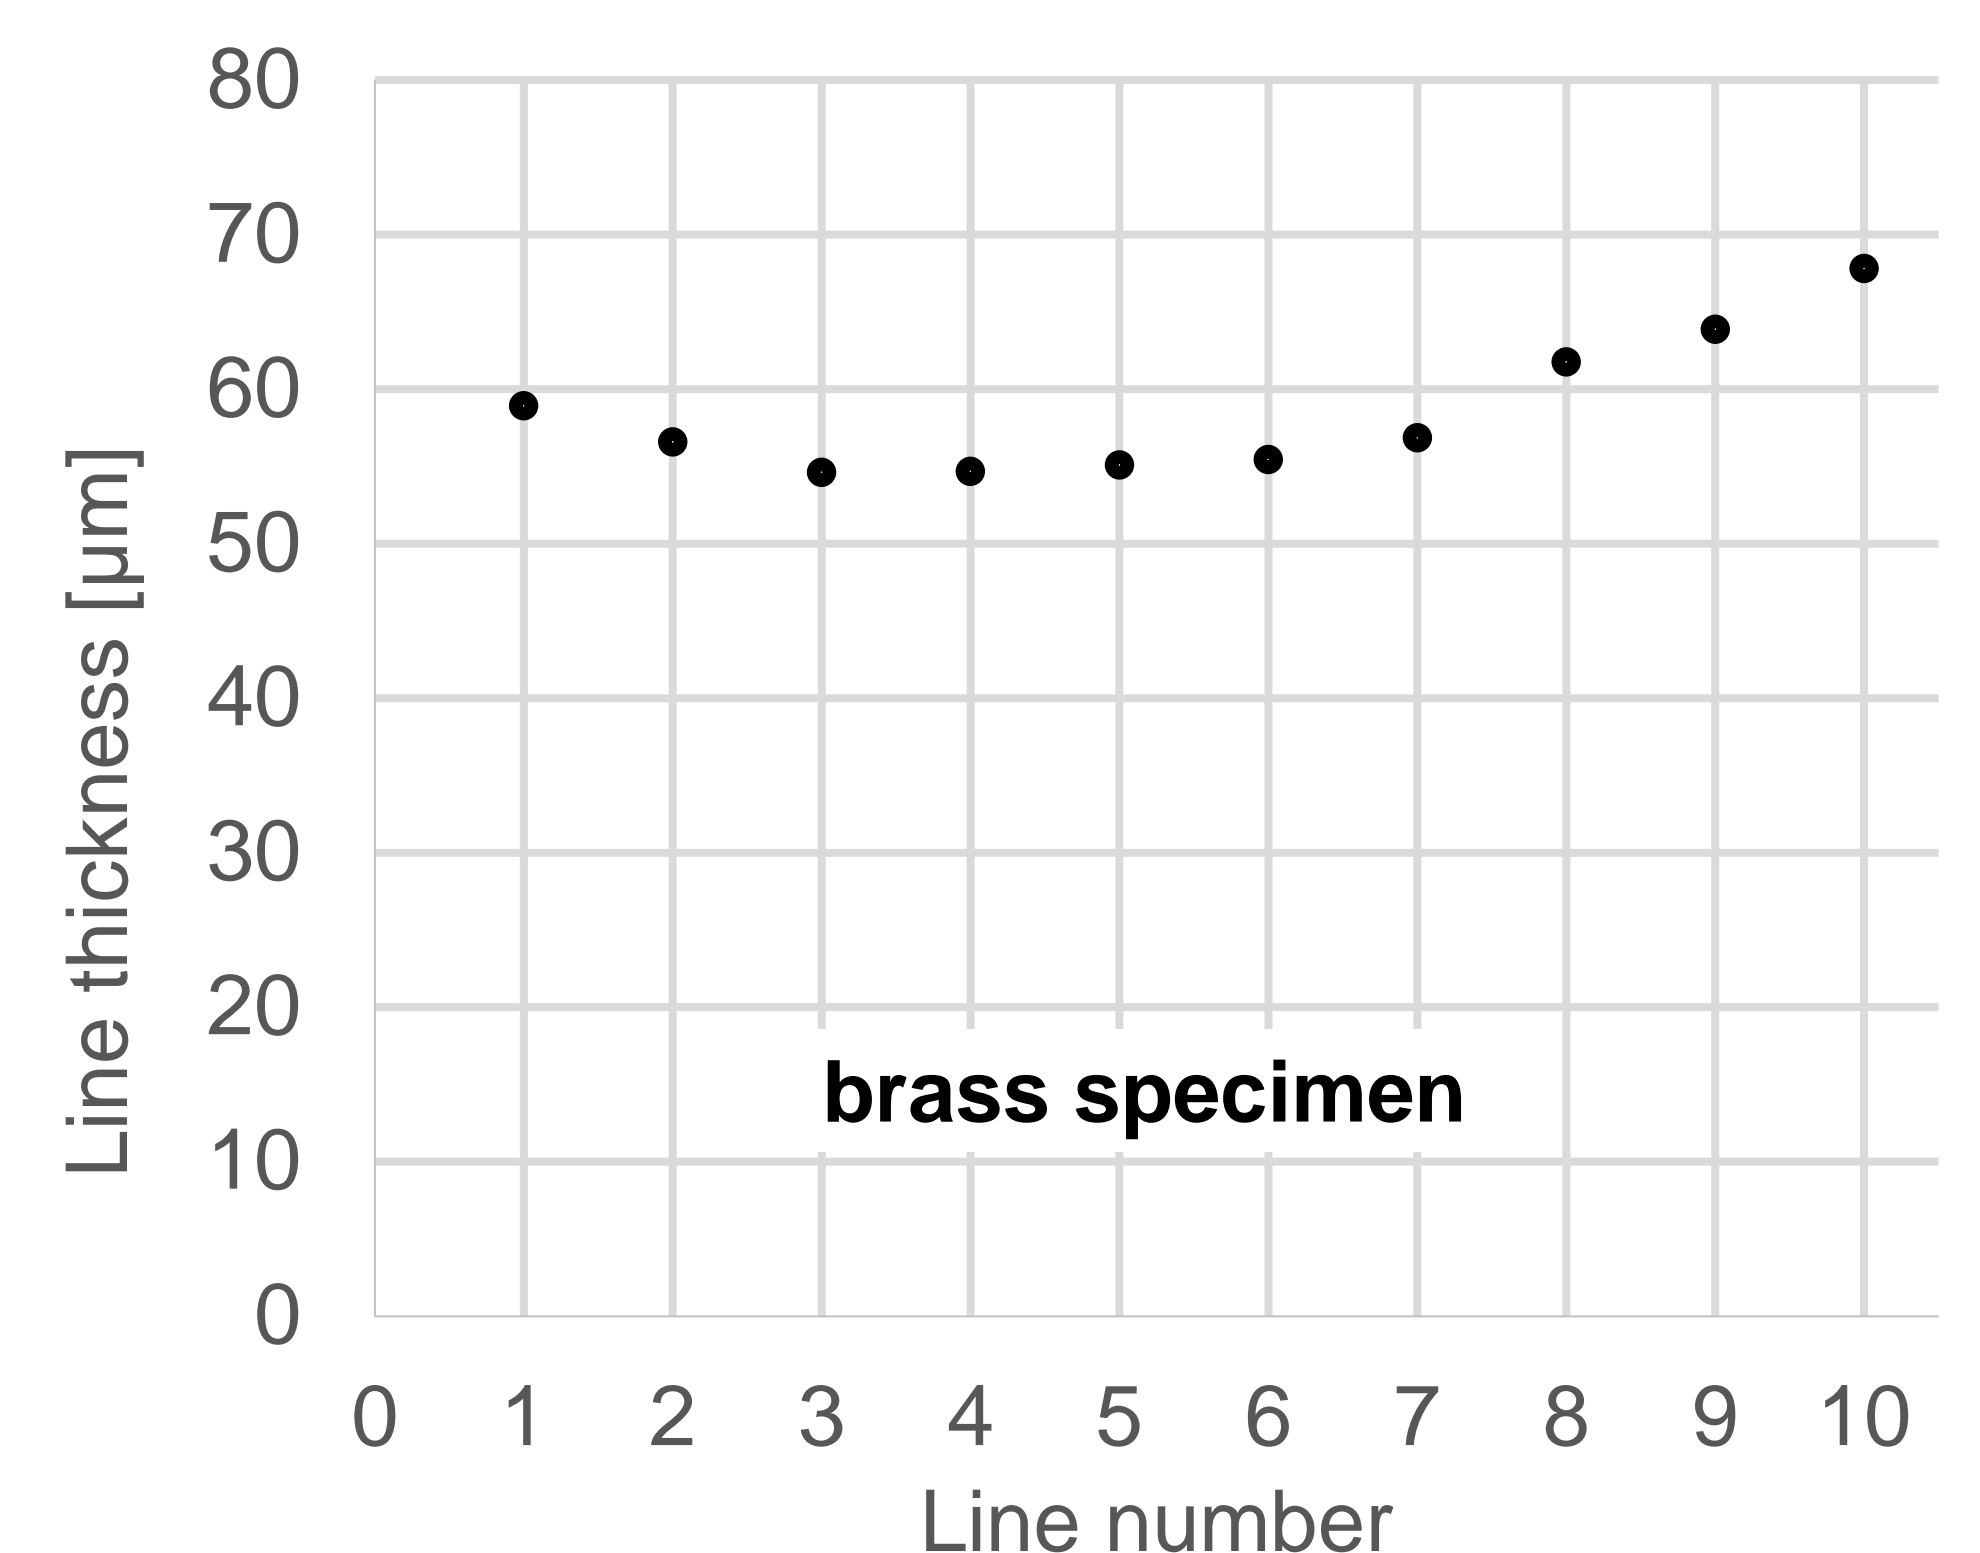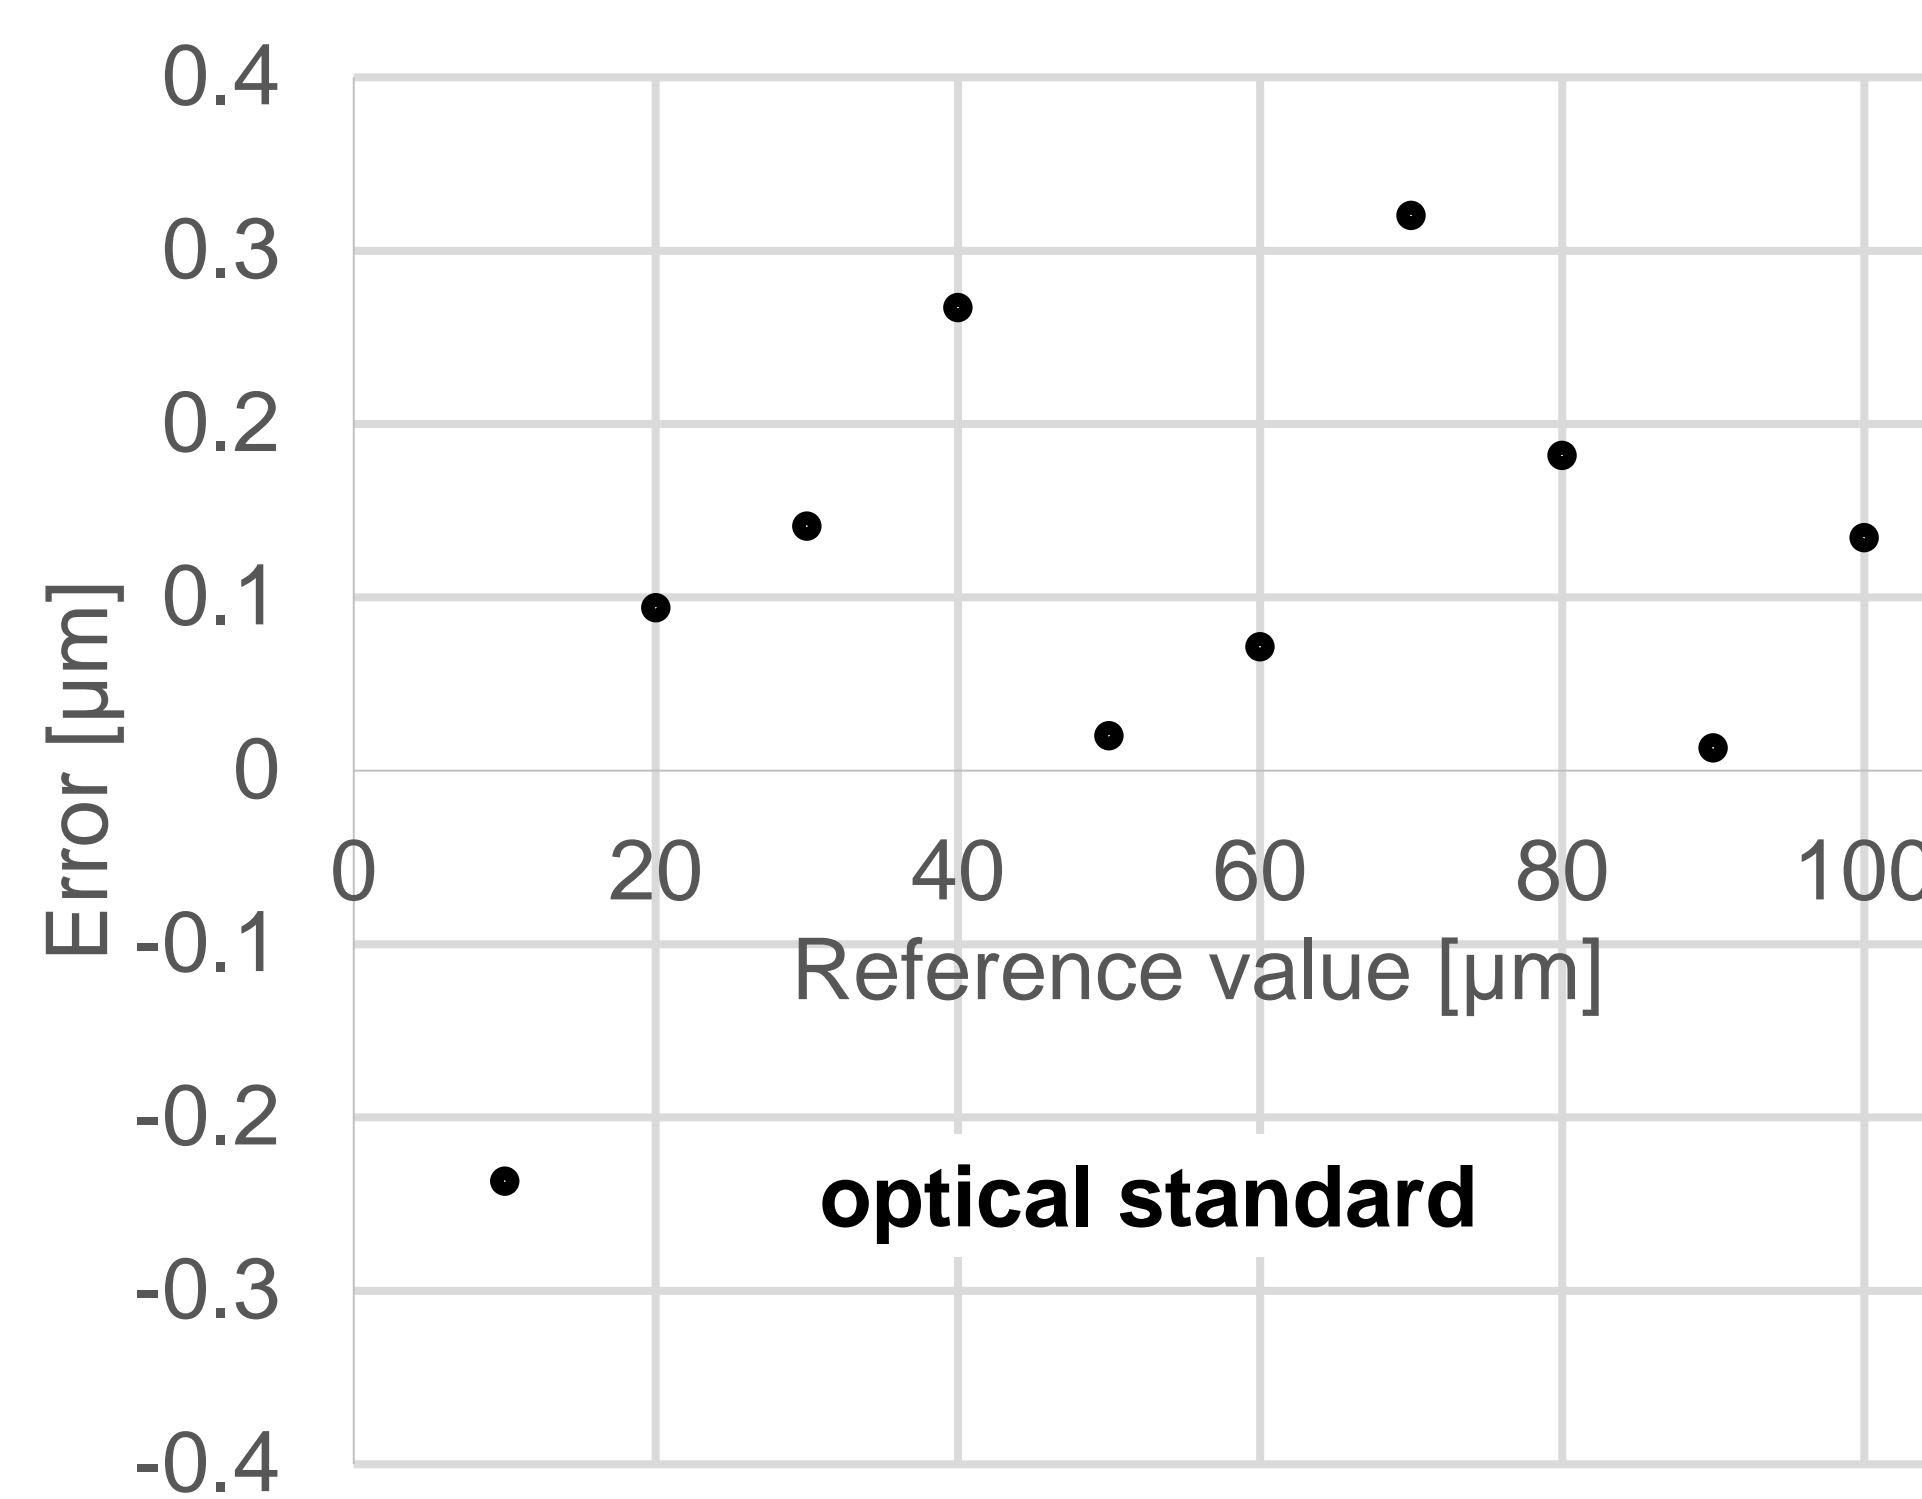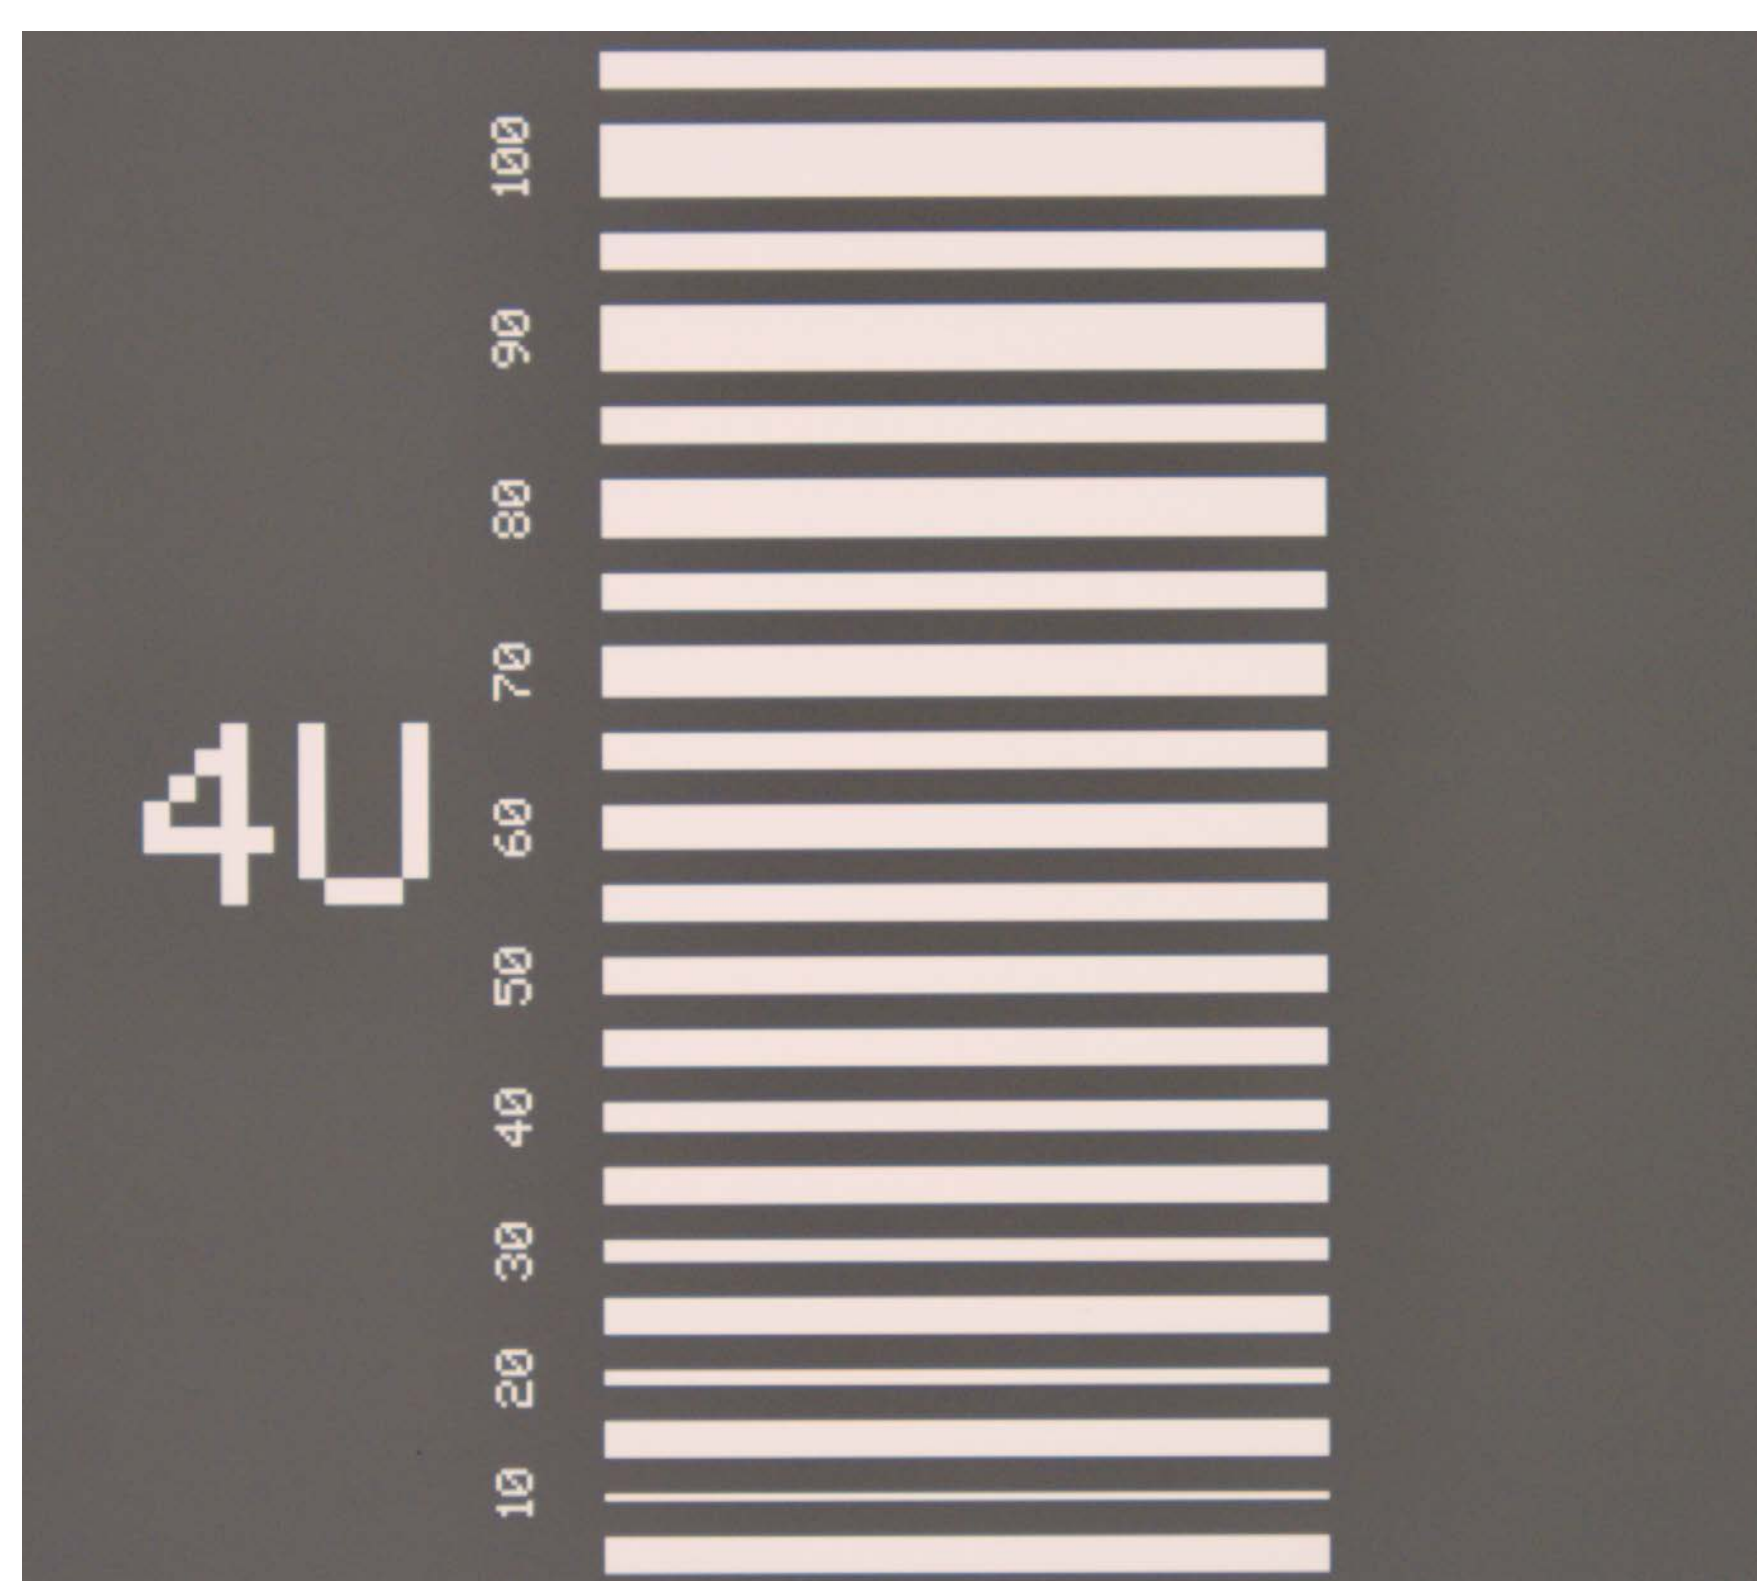

The measurement uncertainty for a single band is calculated as

$$U = k \cdot \sqrt{u_{ref}^2 + u_{rep}^2 + u_p^2 + u_e^2} \text{ where}$$

$u_{ref}$  : reference uncertainty

$u_{rep}$  : uncertainty from repeatability of the measurements on the reference

$u_p$  : specimen line-width uncertainty

$u_e$  : uncertainty coming from the coefficient of thermal expansion

A general expanded uncertainty ( $k=2$ ) of 0.5  $\mu\text{m}$  was estimated for single band measurement on the brass specimen.

The method was applied to quantify the single bands' width and it was observed on the specific item that the bands are slightly wider at the edges, indicating a higher deformation.

Based on the study, it is concluded that the method for automatic measurement of contact areas provides traceable measurements for the investigated dimensional range.