



## Single-photon sources for quantum technologies - Results of the joint research project SIQUTE

Kück, S.; López, M.; Rodiek, B.; Hofer, H.; Porrovecchio, G.; Šmid, M.; Brida, G.; Traina, P.; Degiovanni, I. P.; Pokatilov, A.; Kübarsepp, T.; Manninen, A.; Vaigu, A.; Chunnillal, C.; Szwed, D.; Polyakov, S.; Claudon, J.; Gregersen, Niels; Mørk, Jesper; Chu, X-L.; Götzinger, S.; Lindner, S.; Bock, M.; Becher, C.; Reitzenstein, S.

*Published in:*

Proceedings of 13th International Conference on New Developments and Applications in Optical Radiometry

*Publication date:*  
2017

*Document Version*  
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

*Citation (APA):*

Kück, S., López, M., Rodiek, B., Hofer, H., Porrovecchio, G., Šmid, M., ... Reitzenstein, S. (2017). Single-photon sources for quantum technologies - Results of the joint research project SIQUTE. In Proceedings of 13th International Conference on New Developments and Applications in Optical Radiometry

## DTU Library

Technical Information Center of Denmark

---

### General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

# Single-photon sources for quantum technologies - Results of the joint research project SIQUTE

S. Kück<sup>1</sup>, M. López<sup>1</sup>, B. Rodiek<sup>1</sup>, H. Hofer<sup>1</sup>, G. Porrovecchio<sup>2</sup>, M. Šmid<sup>2</sup>, G. Brida<sup>3</sup>, P. Traina<sup>3</sup>, I. P. Degiovanni<sup>3</sup>, A. Pokatilov<sup>4</sup>, T. Kübarsepp<sup>4</sup>, A. Manninen<sup>5</sup>, A. Vaigu<sup>5,6</sup>, C. Chunnillall<sup>7</sup>, D. Szwer<sup>7</sup>, S. Polyakov<sup>8</sup>, J. Claudon<sup>9</sup>, N. Gregersen<sup>10</sup>, J. Mørk<sup>10</sup>, X-L Chu<sup>11</sup>, S. Götzinger<sup>11</sup>, S. Lindner<sup>12</sup>, M. Bock<sup>12</sup>, C. Becher<sup>12</sup>, S. Reitzenstein<sup>13</sup>

<sup>1</sup>Physikalisch-Technische Bundesanstalt (PTB), Bundesallee 100, 38116 Braunschweig, Germany

<sup>2</sup>Cesky Metrologický Institut (CMI), V Botanice 4, 15072 Praha 5, Czech Republic

<sup>3</sup>Istituto Nazionale di Ricerca Metrologica (INRIM), Strada delle Cacce 91, 10135 Torino, Italy

<sup>4</sup>AS Metrosert (Metrosert), Teaduspargi 8, EE-12618, Tallinn, Estonia

<sup>5</sup>VTT Technical Research Centre of Finland Ltd, Centre for Metrology MIKES, Espoo, Finland

<sup>6</sup>Aalto University, Espoo, Finland

<sup>7</sup>National Physical Laboratory (NPL), Hampton Road, Teddington, TW11 0LW, U.K.

<sup>8</sup>The University System of Maryland Foundation (USMF), College Park, MD 20742, USA

<sup>9</sup>Commissariat à l'énergie atom. et aux énerg. altern. (CEA), INAC, SP2M, 17 rue des martyrs, 38054 Grenoble, France

<sup>10</sup>Danmarks Tekniske Universitet (DTU), Ørstedts Plads, Build. 343, 2800 Kgs. Lyngby, Denmark

<sup>11</sup>Friedrich-Alexander-Universität Erlangen – Nürnberg (FAU), Günther-Scharowsky-Str.1, 91058 Erlangen, Germany

<sup>12</sup>Universität des Saarlandes, Fachrichtung 7.2, Campus E2.6, 66123 Saarbrücken, Germany

<sup>13</sup>Institute of Solid State Physics, Technische Universität Berlin, 10623 Berlin, Germany

Corresponding e-mail address: stefan.kueck@ptb.de

**In this presentation, the results of the joint research project “Single-Photon Sources for Quantum Technologies” (SIQUTE) [1] will be presented. The focus will be on the development of absolutely characterized single-photon sources, on the realization of an efficient waveguide-based single-photon source at the telecom wavelengths of 1.3  $\mu\text{m}$  and 1.55  $\mu\text{m}$ , on the implementation of the quantum-enhanced resolution in confocal fluorescence microscopy and on the development of a detector for very low photon fluxes.**

## INTRODUCTION

The aim of the EURAMET joint research project “Single-photon sources for quantum technologies” (SIQUTE) was the development of highly efficient and predictable single-photon sources for a variety of application, amongst others for radiometry at the low photon flux level. The vision was to develop a single-photon source, which would be a new standard for different fields of research and application. European national metrology institutes (NMIs) and universities joined forces for this common effort.

## RESULTS OF THE SIQUTE PROJECT

Within SIQUTE, a variety of results were obtained, which brings quantum technology and especially quantum radiometry further into the scope of the European NMIs. The results obtained within this


project will be presented at the conference, main results are described in the following:

**Absolute single-photon source [2]:** An NV-centre based single-photon source was absolutely characterized and calibrated in terms of wavelength, background, second order correlation function  $g^{(2)}(t)$ , stability and photon flux. The photon flux was measured with a low noise silicon photodiode traceable to the primary standard for optical flux taking into account the absolute spectral power distribution using a calibrated spectroradiometer. In Fig. 1, the spectra of the NV-centre emission are shown, given in absolute photon flux per wavelength  $N_{\text{ph},\lambda}(\lambda)$  and in absolute radiant flux per wavelength  $\Phi_{\lambda}(\lambda)$ .


**Silicon-vacancy (SiV-) centre based single-photon source [3]:** The absolute photon flux of the emission of a SiV-centre in nanodiamond was directly measured with an absolutely calibrated photodetector at photon rates below 100 000 photons per second. A predictable single photon rate was achieved and used for determining the quantum efficiency of an avalanche photodiode (see Fig. 2).

**Waveguide-based single-photon source [4]:** A setup for the generation of single photons in the telecom band based on spontaneous parametric down-conversion (SPDC) was established. The process employed is based on the spontaneous decay of a pump photon at 710 nm into signal and idler photons at 1310 nm and 1550 nm. Very high photon pair rates

up to  $10^7 \text{ s}^{-1}$ , a signal-to-background ratio of approx.  $600 \mu\text{W}^{-1}$  and a heralding efficiency up to 64 % were measured. Measurements of the heralded  $g^{(2)}$ -functions vs. pump power yield an extremely small  $g^{(2)}(t=0) = 0.001$  at 20 nW pump power, only limited by detector dark counts. Furthermore, the photon indistinguishability was measured in a Hong-Ou-Mandel (HOM) interference experiment. The visibility was measured as a function of the pump power and reaches visibilities  $> 90 \%$  for low pump powers due to the absence of detector noise and multi-photon contributions, see Fig. 3.

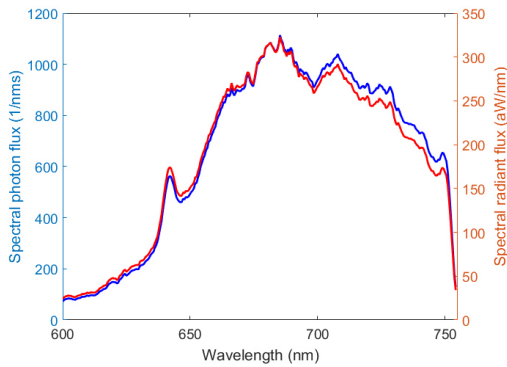

**Figure 1.** Spectra of the NV-centre emission: absolute photon flux per wavelength  $N_{\text{ph},\lambda}(\lambda)$  (blue line) and absolute radiant flux per wavelength  $\Phi_{\lambda}(\lambda)$  (red line).

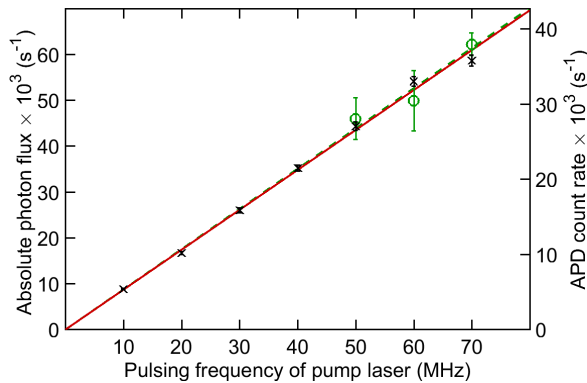


**Figure 2.** Circles: Photon flux measured a calibrated silicon photodetector. Crosses: APD count rates. Straight line: Fit to the data through origin.

Quantum-enhanced resolution [5] was obtained in confocal fluorescence microscopy by exploiting the non-classical photon statistics of single nitrogen-vacancy colour centres in diamond. This was achieved by developing a general model of super-resolution based on the direct sampling of the  $k^{\text{th}}$ -order autocorrelation function of the photoluminescence signal. This model shows that it is possible, in principle, to resolve arbitrarily close emitting single-photon emitters.

Detector development [6]: A transfer standard detector system able to measure 50 fW with an

uncertainty below 1 % at the wavelength range from 650 nm to 750 nm was designed and realized. It consists of a low noise low dark current Si detector (Hamamatsu S1227 33 BR) in conjunction with a custom-made switched integrator amplifier (SIA), which achieves a conversion factor as high as  $10^{12}$ . The noise level measured can be as low as  $1 \text{ fW}/\text{Hz}^{1/2}$  which corresponds to approx. 3500 photons/ $\text{Hz}^{1/2}$  at a wavelength of 750 nm. Allan deviation analysis has shown that a measurement time of 100 s should lead to a standard deviation as low as 400 photons/s.

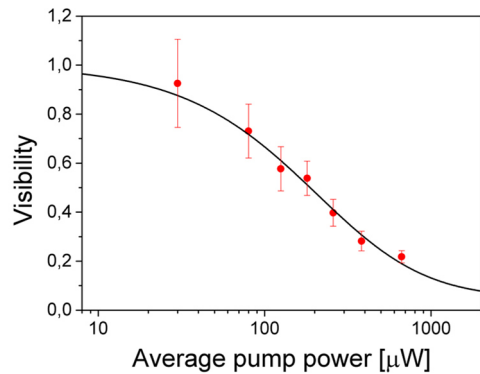

**Figure 3.** Visibility of the HOM dip as a function of average pump power, decreasing towards higher pump powers due to multi-photon contributions.

## SUMMARY

In this contribution, the main achievements of the joint research project SIQUTE were presented.

## ACKNOWLEDGEMENT

This work was funded by the project SIQUTE (contract EXL02) of the European Metrology Research Programme (EMRP). The EMRP is jointly funded by the EMRP participating countries within EURAMET and the European Union.

## REFERENCES

1. <http://www.ptb.de/emrp/siqute.html>
2. B. Rodiek et al., “Experimental realization of an absolute single-photon source based on a single nitrogen vacancy center in a nanodiamond”, *Optica* 4, 71 (2017).
3. A. Vaigu et al., “Tunable and predictable single photon source”, accepted for publication in *Metrologia*.
4. M. Bock et al., “A highly efficient heralded single-photon source for telecom wavelengths based on a PPLN waveguide”, *Optics Express* 24, 23992 (2016).
5. D. Gatto Monticone et al., “Beating the diffraction Abbe limit in confocal microscopy via nonclassical photon statistics”, *Physical Review Letters*, 113, 143602 (2014).
6. G. Porrovecchio et al., “Comparison at the sub-100 fW optical power level of calibrating a single-photon detector using a high-sensitive, low-noise silicon photodiode and the double attenuator technique”, *Metrologia* 53, 1115 (2016).